tryp

Certificate of Analysis


Date:	2025-08-06 13:59:48 -05:00	Cultivar:	
Serial:	LL030614	Moisture:	0.0%
Lab	Tryp Labs	Col Tests Remaining:	12
Operator:	Daniela Tapia	CoA Revision:	0
Sample ID:	Be Cana Vape HHC Mango Blush	Calibration Exp:	2025-12-18
Method:	HPLC	Product:	
Test Type:	Concentrate Hemp Derived	SKU:	
Weight / Volume:	0.109 g	Batch:	
Solvent:	30 ml		
Temperature:	25.5 °C		
Notes:			

Cannabinoid Profile

Analyte	%	LOQ
THC-A	ND	0.91
Δ9-THC	ND	0.91
CBD-A	ND	1.4
CBG-A	ND	1.4
CBD/CBG	ND	1.4
CBN	ND	1.4
CBC	ND	1.4
Δ8-THC*	ND	0.91
Δ10-THC	ND	0.91
THCV	ND	0.91
Δ9-THC-O	ND	2.8
Δ8-THC-O	ND	2.8
HHC	89.4	2.8
Δ9-THCP	ND	2.8
Terpenes	High	
Total THC	**ND**	
Total Cannabinoids	**89.4**	

ND = Not Detected; n/a = Not Analyzed; LOQ = Limit of Quantification; Total THC = (0.877 x THC-A) + Δ9-THC; Total CBD = (0.877 x CBD-A) + CBD. * Δ8THC has lower precision and higher detection limit than other cannabinoids.

Chromatogram

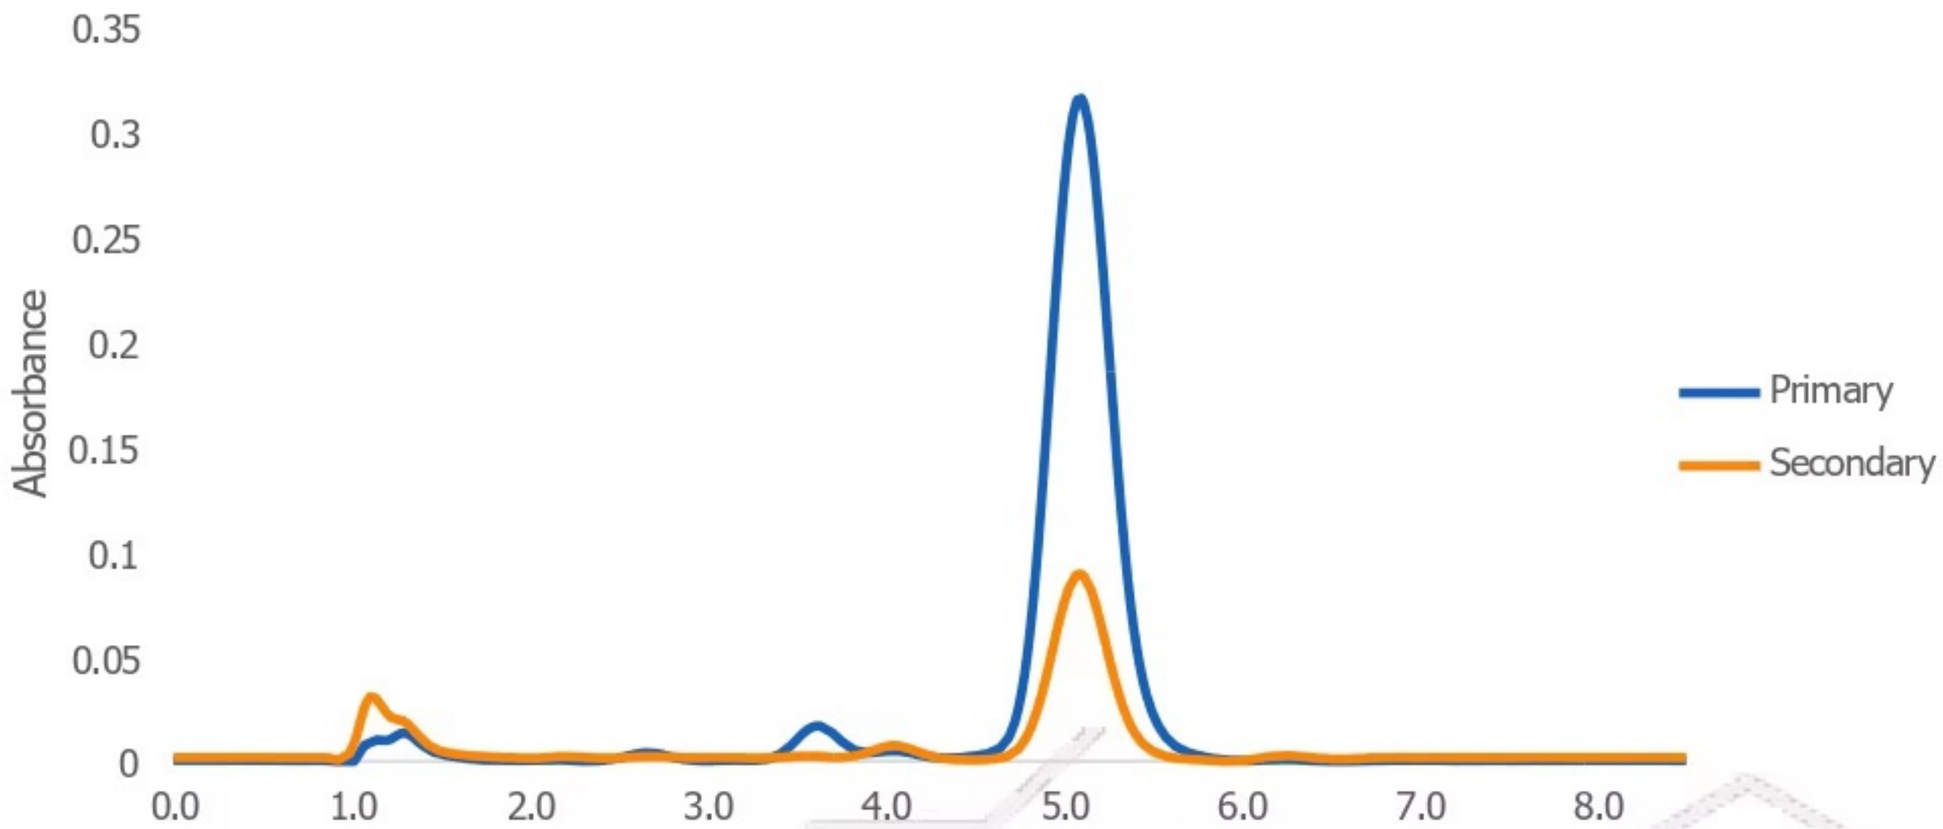

Sample Images



Change History

Date	User	Action
2025-08-06 13:59:48 -05:00		Test Recorded
2025-08-07 11:50:18 -05:00	DT	Added an image
2025-08-07 11:50:29 -05:00		Generated a CoA (revision 0)